

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.

# Advances in quantitative proteomics via stable isotope tagging and mass spectrometry

W Andy Tao and Ruedi Aebersold\*

The high-throughput identification and accurate quantification of proteins are essential components of proteomic strategies for studying cellular functions and processes. Techniques that are largely based on stable isotope protein or peptide labeling and automated tandem mass spectrometry are increasingly being applied in quantitative proteomic studies. Over the past year, significant progress has been made toward improving and diversifying these technologies with respect to the methods for stable isotope labeling, process automation and data processing and analysis. Advances in stable isotope protein labeling and recent biological studies that used stable isotope based quantitative proteomics techniques are reviewed.

## Addresses

Institute for Systems Biology, 1441 North 34th Street, Seattle, WA 98103, USA

\*e-mail: [raebersold@systemsbiology.org](mailto:raebersold@systemsbiology.org)

Current Opinion in Biotechnology 2003, 14:110-118

This review comes from a themed issue on  
Analytical biotechnology  
Edited by Norm Dovichi and Dan Pinkel

0958-1669/03/\$ – see front matter  
© 2003 Elsevier Science Ltd. All rights reserved.

DOI 10.1016/S0958-1669(02)00018-6

## Abbreviations

2DE	two-dimensional gel electrophoresis
CID	collision-induced dissociation
ICAT	isotope-coded affinity tag
MALDI	matrix-assisted laser desorption ionization
MS	mass spectrometry
MS/MS	tandem MS
RPLC	reverse-phase liquid chromatography
RP- $\mu$ LC-MS	reverse-phase microcapillary liquid chromatography coupled on-line with MS

## Introduction

In addition to enumerating the proteins expressed in a species, the detection and quantification of differences in the protein profiles of cells, tissues or body fluids of different origins or states is increasingly being recognized as a key objective of proteomics research. The measurement of differential protein expression provides a more direct, more accurate and more versatile way to detect global changes in cellular dynamics in health and disease compared with the complementary and more mature technology of mRNA expression analysis [1]. Quantitative proteomics thus holds significant promise for the discovery of diagnostic or prognostic protein markers


for the detection of new therapeutic targets and as a powerful tool to further our understanding of basic biological processes and mechanisms. The realization of these expectations relies on the development of automated, robust and highly sensitive methods to identify and quantify proteins.

To date, three different approaches for quantitative protein profiling have been proposed. In the first and most mature approach, proteins are separated and quantified by two-dimensional gel electrophoresis (2DE), and identified by mass spectrometry (MS) [2]. The second approach, protein expression array analysis, is based on the generation of ordered arrays of reagents with high specificity for particular proteins. This method represents the linear translation of the mRNA expression array concept into proteomics and is at present, in spite of its enormous promise, least developed [3]. The third and currently most rapidly advancing approach is based on stable isotope labeling of proteins or peptides and automated tandem mass spectrometry (MS/MS). Chemically identical but mass-differentiated stable isotope tags are introduced into the proteins in two sample mixtures. The combined mixtures are then processed and analyzed by MS so that each analyte from one sample represents a quantitative standard for a chemically identical analyte from the other sample. The isotope tags can optionally contain an affinity tag so that the tagged analytes can be selectively isolated, thus simplifying the complexity of sample mixtures before mass-spectrometric analysis. This review summarizes recent advances in quantitative proteomics technology based on stable isotope tagging and MS/MS and discusses results from selected applications.

## Current status and applications of quantitative proteomics using stable isotope tags and mass spectrometry

The prototypical method to generate quantitative protein profiles based on stable isotope affinity tagging and MS is the isotope-coded affinity tag (ICAT) reagent method [4]. The reagents (Figure 1) consist of a cysteine-reactive group, a linker that contains either heavy or light isotopes, and a biotin affinity tag. The ICAT reagent method (Figure 2) involves *in vitro* derivatization of cysteine residues with the isotopically heavy or light form of the reagent, respectively, then enzymatic digestion of the combined sample and isolation and mass spectrometric analysis of labeled peptides [4]. In the process the complexity of the peptide sample mixture is significantly reduced and each peptide is isotopically tagged to facilitate quantitative mass spectrometric measurements.

Figure 1




The structure of ICAT reagents. ICAT reagents comprise a cysteine-reactive group, a linker containing either heavy or light isotopes and a binding affinity tag.

Results from a series of applications of the method have illustrated its versatility, documented current technical limitations and showed new uses for quantitative proteomic analyses. The applications can be broadly grouped into three classes, as detailed below. In the first, quanti-

tative proteomics was used to ask whether the analysis of perturbation-induced changes measured at the mRNA and protein levels provide redundant or complementary information. In the second class, quantitative proteomics was used to gain new insights into specific cellular

Figure 2

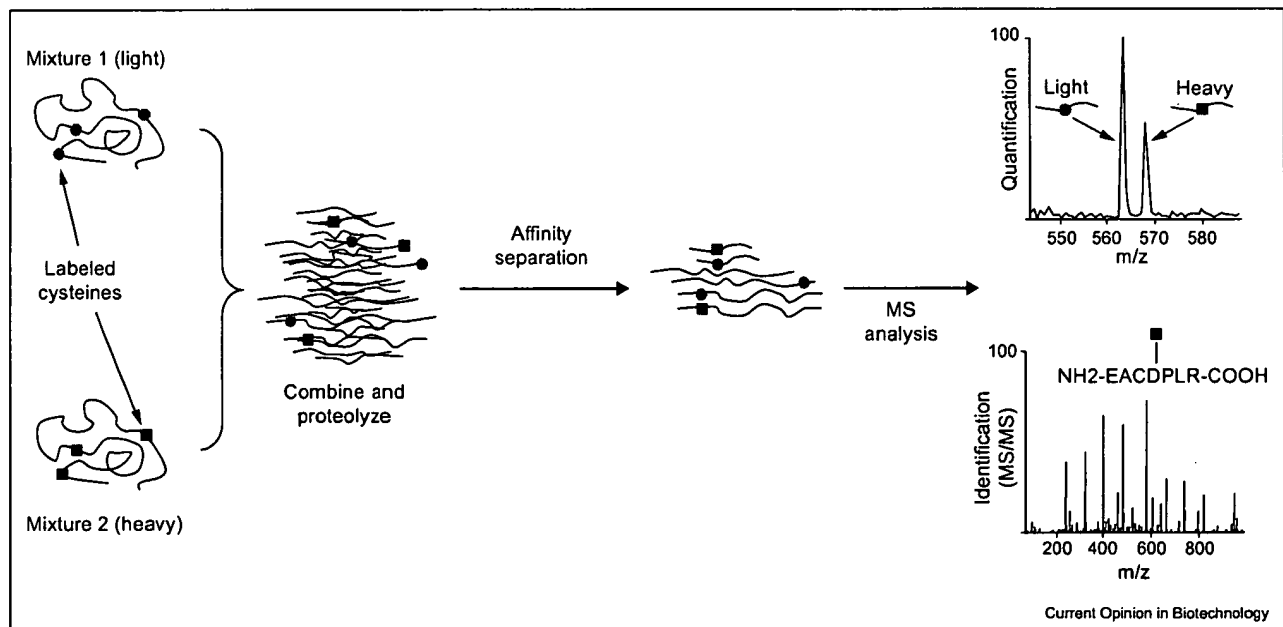

The ICAT reagent strategy for quantifying differential proteins. Two protein mixtures representing two different cell states are treated with the isotopically light (green) or heavy (red) ICAT reagents, respectively. The labeled protein mixtures are then combined and proteolyzed; tagged peptides are selectively isolated and analyzed by MS. The relative abundance is determined by the ratio of signal intensities of the tagged peptide pairs. Every other scan is devoted to fragmenting a peptide. The CID spectra are recorded and searched against large protein sequence databases to identify the protein. Therefore, in a single operation, the relative abundance and sequence of a peptide are determined.

mechanisms (e.g. specific signaling mechanisms). In the third class, applications that use quantitative proteomics for purposes that go beyond simple protein profiling were explored.

#### Are the measurement of the cellular response to external perturbations at the mRNA and protein level redundant or complementary?


A main objective of the emerging 'Systems Biology' approach is to use different types of systematic and quantitative measurements to dissect the complex systems and networks that underlay cell physiology [5]. To date, the types of data most commonly acquired in this context are mRNA expression profiles and protein expression profiles. Several studies examined the important question of whether the information obtained from studying the responses of a system to external perturbations measured at the mRNA and protein level is redundant or complementary.

In the first such study the responses of cells of the yeast *Saccharomyces cerevisiae* to perturbations along the extensively studied galactose utilization pathway were analyzed using full-genome cDNA microarrays and quantitative proteomics via the ICAT reagent method [6\*\*]. The protein-abundance ratios of 289 proteins were determined for wild-type cells grown in the presence (+gal) or absence (-gal) of 2% galactose and related to the correspond-

ing mRNA expression ratios. The results, reproduced in Figure 3, indicate a loose positive correlation between the two types of data. More interestingly, the data also suggested that the expression of 15 proteins involved post-transcriptional regulation and that groups of functionally related genes showed similar expression patterns. This is exemplified by the observation that the mRNA levels of several ribosomal proteins increased three- to five-fold in response to galactose addition, whereas the corresponding protein abundances remained unchanged.

A similar study investigated the effects of carbon-source perturbation on steady-state gene expression in *S. cerevisiae*. The cells were grown in galactose or ethanol and the induced changes in mRNA and protein profiles were measured and correlated [7]. For genes involved in glycolysis, the response measured at the mRNA and protein levels correlated well, whereas for mitochondrial proteins involved in energy metabolism and for proteins involved in protein synthesis, significant discrepancies in expression ratios were observed. Using 2DE-MS and gene expression arrays, respectively, to study the activation of human neutrophils by lipopolysaccharide at the protein and mRNA levels, Fessler and co-workers [8\*] also found generally poor correlation between the datasets. Collectively, these results emphasize the importance of integrated mRNA and protein expression measurements for understanding biological systems.

Figure 3



Scatter plot of protein expression ratios versus mRNA expression ratios. Ratios of protein expression for 289 proteins were determined using the ICAT technique. The values are plotted against the corresponding mRNA expression ratios measured by full-genome microarrays. Many metabolic (blue triangles) or ribosomal (green diamonds) proteins were elevated in wild type + gal, while those involved in respiration (red triangles) had reduced expression levels. Names of genes that were indistinguishable in both mRNA and protein expression are separated by a slash (from [6\*\*]).

### Insights into specific signaling mechanisms

Specific signaling pathways have traditionally been studied at the protein level using antibody-based approaches including western blots, enzyme-linked immunosorbent assays, immunoprecipitation of signaling complexes and immunohistochemistry. Although these methods are extremely sensitive and specific, the reliance on high quality antibodies precludes quick and high-throughput analyses and limits the generality of the approach. Furthermore, an antibody that binds a native protein may not be useful for detecting the denatured protein on a western blot and antibody-based methods necessarily anticipate the events that are being assayed and are blind to unexpected events. The ability of quantitative proteomics technologies to compare the expression levels of hundreds-to-thousands of proteins in cells of different states of activation promises new insights into the mechanism of specific signaling pathways and, more importantly, into the interconnection between different signaling systems.

These expectations were realized by a study in which the ICAT reagent method was applied to investigate the function of the Myc oncoprotein [9\*]. By comparing the global pattern of protein expression between *myc*-null and *myc*-plus cells, groups of functionally diverse proteins were identified as being regulated by the presence or absence of Myc. These included those predicted to lead to increased cell growth, reduced focal adhesions, as well as altered morphology. A novel cytoskeletal function of Myc was revealed using this approach, indicating the feasibility of quantitative whole-proteome analysis in mammalian cells to understand the molecular functions of pleiotropic regulators such as Myc. Using the same experimental strategy, Han *et al.* [10] identified an unprecedented number of microsomal proteins and determined their quantitative response to the pharmacologically induced differentiation in human myeloid leukemia (HL-60) cells; Smith and co-workers [11] identified and quantified changes in protein expression between control and camptothecin-treated mouse cortical neurons; and Baliga and co-workers [12] studied the regulatory networks underlying the shift of the extremely halophilic *Halobacterium* from aerobic to anaerobic phototrophic energy production. These studies indicate that quantitative proteomics can provide new insights into the molecular mechanisms that control diverse physiological functions in prokaryotic or eukaryotic cells.

### Beyond profiling

Most cellular functions are not performed by individual proteins but rather by complexes of interacting proteins. It is therefore an important component of quantitative proteomics to identify specifically interacting proteins and to determine differences in the composition of protein complexes isolated from different cellular sources.

A generic strategy to characterize partially purified macromolecular complexes using the ICAT reagent method has been presented (JA Ranish *et al.*, unpublished results). The principle of the method is schematically illustrated in Figure 4. By comparing the relative abundance of peptides from a control sample that does not contain the target complex and a sample that contains the target complex within a matrix of proteins unrelated to the complex, the specific complex components can be identified on the basis of the enrichment factor observed between the two samples. The method was applied to study the large RNA polymerase II pre-initiation complex from yeast cells that was purified from nuclear extracts by a single-step promoter DNA affinity procedure. In a single experiment, 45 of the 49 known components of the complex were identified within a background of 206 contaminating proteins, illustrating the power of quantitative proteomics technology for the characterization of protein complexes.

Stable isotope labeling in combination with the  $\beta$ -elimination of *O*-phosphate was also proposed for the quantitative analysis of phosphopeptides [13]. The study addressed an issue of central importance for proteomics — the comprehensive and quantitative analysis of cellular protein phosphorylation profiles. The study also illustrated the remaining substantial challenges facing systematic protein phosphorylation analysis, including the diverse chemical nature of the phosphate-ester bonds occurring on proteins, difficulties in detecting phosphorylation events in low abundance proteins, and the potential of other groups to undergo  $\beta$ -elimination, thus complicating the interpretation of mass spectra obtained from such experiments.

Rather than analyzing global protein profiles, in what they termed the 'mass western method', Arnott and co-workers used quantitative proteomics technology based on stable isotope tagging to selectively detect the presence of the cell-surface proteins prostate stem cell antigen (PSCA) and ErbB2 and to determine their relative abundance in different cell lines [14\*]. This method obviates the need for gel electrophoresis or other initial purification steps.

These examples illustrate that proteomics technologies based on stable isotope labeling and quantitative MS are being used in creative experiments to measure biologically informative properties of the proteome that are beyond the sequence and quantity of expressed polypeptides.


## Technical advances

### Chemistry

#### New isotope-coded affinity-tagged reagents

Early applications of the ICAT reagent method identified several drawbacks of the first-generation reagents. First,

Figure 4

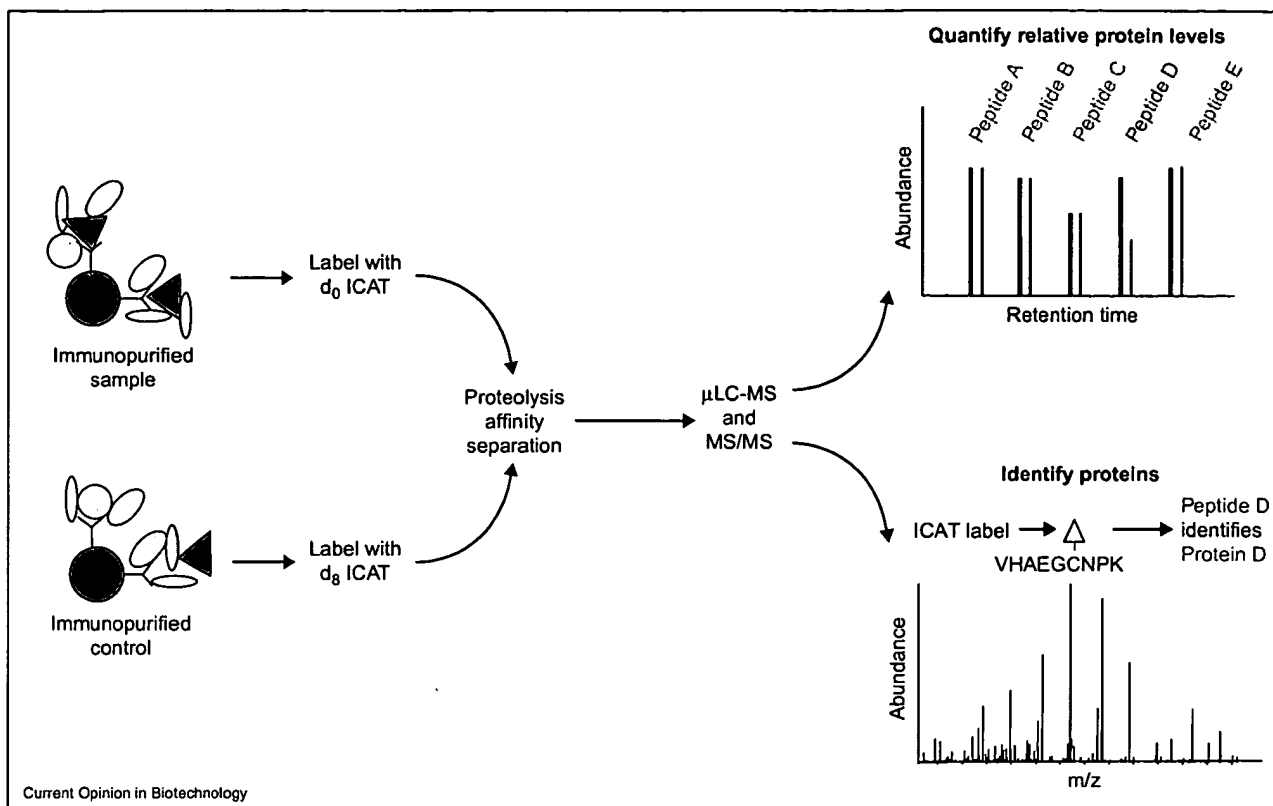


Quantitative proteomics approach for the analysis of affinity-purified macromolecular complexes. To distinguish specific complex components from copurifying proteins, a control purification is performed in which the complex of interest is not enriched. Proteins purified by immunoprecipitation from sample and control are labeled with either the isotopically heavy or light version of the ICAT reagent, and combined. After proteolysis, sample complexity is reduced in three sequential chromatographic steps, and the peptides are analyzed by ESI-MS/MS to obtain their identity and quantity. The relative quantification can then be used to distinguish specific complex components from copurifying proteins.

the combined biotin-isotope tag is relatively large and bulky. As the tag remains on each peptide during MS analysis it is also subject to fragmentation under collision-induced dissociation (CID) conditions and the resulting tag-specific fragment ions can complicate the manual or computer-assisted interpretation of tandem mass spectra of labeled peptides. Second, the eight deuterium atoms that were used as the mass-tags in the original ICAT reagents caused an isotope effect that was sufficient to partially resolve isotopic peptide pairs by high-resolution reverse-phase liquid chromatography (RPLC) [15<sup>\*</sup>]. Therefore, accurate quantification requires the calculation of the abundance ratios on the basis of the integrated peak areas of the heavy and light forms of each peptide, complicating automated data analysis [10].

To address these issues, several second-generation chemistries for cysteine-specific isotope tagging have been developed. Zhou and co-workers [16<sup>\*</sup>] described a method that uses solid-phase capture-and-release to introduce stable isotope tags at cysteine residues and to isolate the

tagged peptides. The solid-phase resin was prepared by modifying the surface of controlled pore glass beads with a chemical structure consisting of a photo-cleavable linker, an isotope-tag transfer group and a specific reactive group (Figure 5). Using Fmoc peptide synthesis chemistry two types of beads were synthesized with surface modifications that were chemically identical but differed in the isotopic composition of the tag.

Compared with the solution-phase ICAT reagent method, the solid-phase tag transfer method has several advantages. First, as the isolation of cysteine-containing peptides and incorporation of stable isotopes are achieved in a single step, the solid-phase method is faster and simpler, requires less manual input and is easier to automate. Second, stringent wash conditions are compatible with the covalent capture of peptides, resulting in the recovery of a sample mixture highly enriched for cysteine-containing peptides. Third, no additional steps are needed to remove reagents. Fourth, the minimal number of sample handling steps increases the sensitivity



**Structure of reagents for solid-phase isotope tag transfer.**

A similar solid-phase approach using an acid-labile resin has also been described [17<sup>+</sup>] and Applied Biosystems, Inc. (Foster City, CA) recently introduced a new version of ICAT reagents that contain an acid-cleavable linker between the isotope tag and the biotin group [18<sup>+</sup>]. Peptides labeled with the second-generation ICAT reagents are subjected to the same separation procedures as those labeled with the original version of the reagent, except that as an additional step the biotin group is cleaved off before MS analysis of the tagged peptides. The isotope tag introduced with this reagent consists of <sup>13</sup>C instead of deuterium and is relatively small. As expected [15<sup>+</sup>] the peptides labeled with the <sup>13</sup>C<sub>6</sub> or <sup>12</sup>C<sub>6</sub> isotope tag have virtually the same retention time during RPLC.

Thiol-specific reagents have the advantage that they selectively isolate cysteine-containing peptides from a complex sample mixture and therefore reduce the complexity of the sample to be analyzed by MS. The reagents have the disadvantage that proteins that do not contain any cysteines are transparent to the method and that generally relatively low sequence coverage of the identified proteins is achieved. In an attempt to isotopically label every peptide in a protein digest, N-terminal label-

### Enzyme-catalyzed $^{18}\text{O}$ and metabolic stable isotope labeling

Apart from chemical and enzymatic methods, metabolic protein labeling has also been used to introduce stable tags into proteins for quantitative proteomics. Whereas in the past metabolic stable isotope labeling was achieved by using culture media containing salts that were isotopically enriched [29–31], or depleted [31,32], more recently proteins were also labeled via the metabolic incorporation of ‘heavy’ amino acids [33\*,34–36]. These advances provide the opportunity to also perform metabolic labeling in cultured mammalian cells. The labeling of proteins in whole higher organisms remains, however, beyond the reach of metabolic stable isotope labeling methods.

A method that is conceptually analogous to the ICAT reagent labeling method but does not make use of stable isotopes was described by Cagney and Emili [37]. The method, termed mass-coded abundance tagging (MCAT), relies on the selective and quantitative guanidination of the  $\epsilon$ -amino group of C-terminal lysine residues of tryptic peptides and thus the transformation of lysines into homoarginine. After differential modification of tryptic peptides contained in one sample and the combination of the tagged peptides with the untagged peptides in a second sample, the relative abundance of each peptide contained in the two samples can be estimated by mea-

asuring the relative signal intensities of each sister peptide pair in full-scan MS mode. The relatively large mass difference (42 Da) between unmodified and modified peptides and the potential for partial modification of the  $\alpha$ -amino groups during the guanidination reaction potentially complicate the MCAT approach for the analysis of very complex mixtures.

#### Data acquisition and instrumentation


To date, most analyses based on the ICAT reagents or related methods have been carried out using reverse-phase microcapillary liquid chromatography coupled on-line with MS (RP- $\mu$ LC MS) and RP- $\mu$ LC MS/MS. In such experiments, peptides at specific mass-to-charge ( $m/z$ ) values are selected for CID using a data-dependent software routine with dynamic exclusion and are identified by searching the resulting CID spectra against a protein sequence database. The abundance ratio is then determined for each identified peptide. Usually a routine of alternating MS and MS/MS scans is used to collect both qualitative and quantitative data in the same experiment.

Further developments have been made on improving peptide identification and accurate quantification. One such case is the establishment of an empirical statistical model to estimate the accuracy of peptide identifications assigned to CID spectra made by database search applications [38]. The model computes probabilities that

peptide assignments to spectra are correct on the basis of database search scores, providing a particularly useful criterion for distinguishing correctly from incorrectly assigned peptides. It also has become apparent that the fact that the analytes contain isotopic signatures can be used to adapt the MS strategies for their analysis. An early example of such an adaptation is the development of instrument control protocols in a matrix-assisted laser desorption ionization ESI electrospray ionization (MALDI) quadrupole time-of-flight MS (QqTOF) instrument that automatically selects precursor ions on the basis of abundance ratio of detected, isotopically labeled peptide pairs [39]. The rationale for the method is the observation that in most proteomic experiments that compare perturbed cellular states, the abundance of the majority of the detected proteins remains unchanged. The described protocol therefore focuses the mass spectrometer on those peptides that show a difference in expression, that is, the biologically most informative species.

The use of MALDI-MS/MS offers the significant advantage that the temporal constraints of on-line detection that are typically encountered with ESI-MS/MS are eliminated as the peptides separated by  $\mu$ LC are deposited on a MALDI sample plate before MS analysis. It can be expected that the absence of this temporal constraint will catalyze the development of further MS and MS/MS

Figure 6

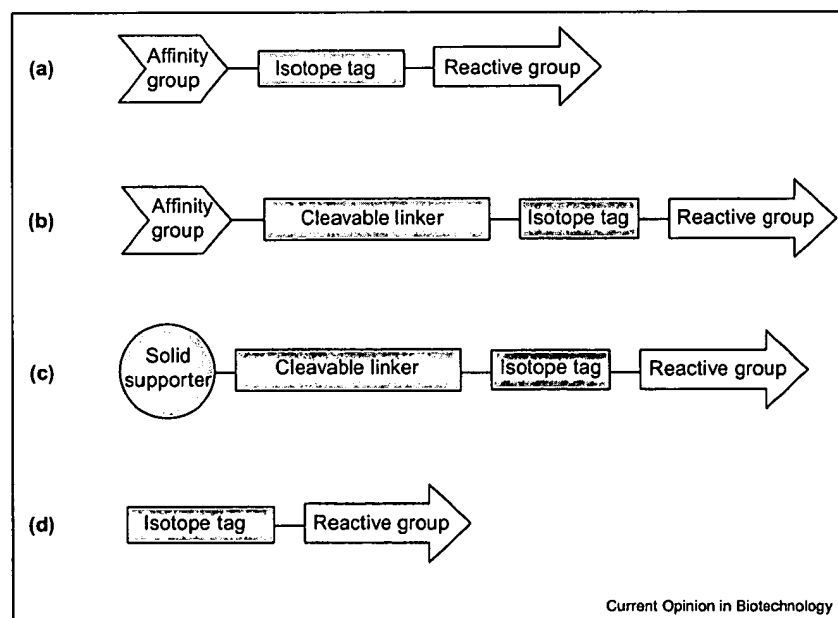

Summary of available isotope tagging reagents. (a) Classical ICAT reagents that contain an affinity group, an isotope linker, and a reactive group. (b) Cleavable ICAT reagents that have an additional cleavable linker between affinity group and isotope tag; both (a) and (b) reagents are suitable for solution-phase derivatization of cysteine residues on proteins. (c) Reagents for stable isotope tag transfer via solid-phase capture and release. (d) Reagents that introduce a stable isotope tag on peptides.



protocols that focus on selected proteins of great biological significance, a trend that will surely be accelerated by the availability of new types of MALDI MS/MS instruments such as the MALDI-TOF-TOF (MALDI tandem time-of-flight) [40–43].

## Conclusions

With steady advances in chemistry (summarized in Figure 6), instrumentation and reference tools for the generation of stable isotope tagged polypeptides and their analyses, quantitative proteomics is poised to realize its immense potential for basic and clinical research. Fully robotized, high-throughput platforms, robust isotope tagging chemistries with different selectivities, improved transparent, probability-based data analysis tools and optimized interfaces between the analytical platforms and the biological specimens remain significant challenges facing the proteomics field. It can be expected that current and emerging proteomic approaches will find applications to various biological systems [44,45] and that the coming years will demonstrate their enormous utility for drug discovery, disease prevention and diagnosis and basic biological research.

## Acknowledgements

This work was supported by grants from the National Cancer Institute (NCI) (R33, CA 93302), National Heart Lung and Blood Institute (NHBLI), Proteomics Initiative (N01-HV-28179), National Institute on Drug Abuse (NIDA) (P30, DA 15625), and a grant from Oxford GlycoScience. The ISB is supported by a generous gift from Merck and Co. WAT is a Damon Runyon Fellow supported by the Damon Runyon Cancer Research Foundation (DRG 1740-02).

## References and recommended reading

Papers of particular interest, published within the annual period of review, have been highlighted as:

- of special interest
- of outstanding interest

1. Duggan DJ, Bittner M, Chen Y, Meltzer P, Trent JM: **Expression profiling using cDNA microarrays.** *Nat Genet* 1999, 21:10–14.
2. Aebersold R, Goodlett DR: **Mass spectrometry in proteomics.** *Chem Rev* 2001, 101:269–295.
3. Jenkins RE, Pennington SR: **Arrays for protein expression profiling: towards a viable alternative to two-dimensional gel electrophoresis?** *Proteomics* 2001, 1:13–29.
4. Gygi SP, Rist B, Gerber SA, Turecek F, Gelb MH, Aebersold R: **Quantitative analysis of complex protein mixtures using isotope-coded affinity tags.** *Nat Biotechnol* 1999, 17:994–999.
5. Ideker T, Galitski T, Hood L: **A new approach to decoding life: systems biology.** *Annu Rev Genomics Hum Genet* 2001, 2:343–372.
6. Ideker T, Thorsson V, Ranish JA, Christmas R, Buhler J, Eng JK, • Bumgarner R, Goodlett DR, Aebersold R, Hood L: **Integrated genomic and proteomic analyses of a systematically perturbed metabolic network.** *Science* 2001, 292:929–934.
- A pilot study demonstrating the Systems Biology approach that integrates quantitative data, at both the genomic and proteomic levels.
7. Griffin TJ, Gygi SP, Ideker T, Rist B, Eng J, Hood L, Aebersold R: **Complementary profiling of gene expression at the transcriptome and proteome levels in *Saccharomyces cerevisiae*.** *Mol Cell Proteomics* 2002, 1:323–333.
8. Fessler MB, Malcolm KC, Duncan MW, Worthen GS: **A genomic and proteomic analysis of activation of the human neutrophil by lipopolysaccharide and its mediation by p38 mitogen-activated protein kinase.** *J Biol Chem* 2002, 277:31291–31302.
- The authors demonstrate that the measurements of the cellular response to external perturbations at the mRNA and protein levels are complementary in mammalian cells.
9. Shiio Y, Donohoe S, Yi EC, Goodlett DR, Aebersold R, Eisenman • RN: **Quantitative proteomic analysis of Myc oncoprotein function.** *EMBO J* 2002, 21:5088–5096.
- Description of a novel quantitative proteomic approach to the analysis of Myc oncoprotein function, indicating the feasibility of quantitative whole-proteome analysis in mammalian cells.
10. Han DK, Eng J, Zhou H, Aebersold R: **Quantitative profiling of differentiation-induced microsomal proteins using isotope-coded affinity tags and mass spectrometry.** *Nat Biotechnol* 2001, 19:946–951.
11. Yu LR, Johnson MD, Conrads TP, Smith RD, Morrison RS, Veenstra TD: **Proteome analysis of camptothecin-treated cortical neurons using isotope-coded affinity tags.** *Electrophoresis* 2002, 23:1591–1598.
12. Baliga NS, Pan M, Goo YA, Yi EC, Goodlett DR, Dimitrov K, Shannon P, Aebersold R, Ng WV, Hood L: **Coordinate regulation of energy transduction modules in *Halobacterium* sp. analyzed by a global systems approach.** *Proc Natl Acad Sci USA* 2002, 99:14913–14918.
13. Goshe MB, Veenstra TD, Panisko EA, Conrads TP, Angell NH, Smith RD: **Phosphoprotein isotope-coded affinity tags: application to the enrichment and identification of low-abundance phosphoproteins.** *Anal Chem* 2002, 74:607–616.
14. Amott D, Kishiyama A, Luis EA, Ludlum SG, Marsters JC Jr, Stults • JT: **Selective detection of membrane proteins without antibodies: a mass spectrometric version of the western blot.** *Mol Cell Proteomics* 2002, 1:148–156.
- The paper has used the isotope-tagging technology for a novel approach. Rather than analysing global protein profiles, the technology has been used to monitor several important cell surface proteins in prostate cells.
15. Zhang R, Sioma CS, Wang S, Regnier FE: **Fractionation of isotypically labeled peptides in quantitative proteomics.** *Anal Chem* 2001, 73:5142–5149.
- The authors have recognized potential resolution of isotopic forms of a peptide on reverse-phase chromatography and its resulting inconvenience in quantitative proteomics.
16. Zhou H, Ranish JA, Watts JD, Aebersold R: **Quantitative proteome analysis by solid-phase isotope tagging and mass spectrometry.** *Nat Biotechnol* 2002, 20:512–515.
- See annotation to [18].
17. Qiu Y, Sousa EA, Hewick RM, Wang JH: **Acid-labile isotope-coded extractants: a class of reagents for quantitative mass spectrometric analysis of complex protein mixtures.** *Anal Chem* 2002, 74:4969–4979.
- A solid-phase version of ICAT reagents was introduced in both papers [17,18]. As a significant step toward the development of new quantitative proteomics reagents, the solid-phase approach facilitates fully robotized, high-throughput quantitative proteomic analysis.
18. Juhasz P, Falick A, Graber A, Hattan S, Khainovski N, Marchese J, Martin S, Patterson D, Williamson B, Malmstrom J et al.: **ESI and MALDI/MS-MS approaches for large scale protein identification and quantification: are they equivalent? 50th American Society for Mass Spectrometry Conference June 2–6, 2002, Orlando, FL.**
- New ICAT reagents, acid cleavable ICAT reagents, were introduced. Studies with the new reagents indicate better identification and quantification for proteomic analysis.
19. Munchbach M, Quadroni M, Miotto G, James P: **Quantitation and facilitated *de novo* sequencing of proteins by isotopic N-terminal labeling of peptides with a fragmentation-directing moiety.** *Anal Chem* 2000, 72:4047–4057.
20. Chakraborty A, Regnier FE: **Global internal standard technology for comparative proteomics.** *J Chromatogr A* 2002, 949:173–184.
21. Wang S, Zhang X, Regnier FE: **Quantitative proteomics strategy involving the selection of peptides containing both cysteine and histidine from tryptic digests of cell lysates.** *J Chromatogr A* 2002, 949:153–162.

22. Amini A, Chakraborty A, Regnier FE: **Simplification of complex tryptic digests for capillary electrophoresis by affinity selection of histidine-containing peptides with immobilised metal ion affinity chromatography.** *J Chromatogr B Analyt Technol Biomed Life Sci* 2002, **772**:35-44.
  23. Zhou H, Watts JD, Aebersold R: **A systematic approach to the analysis of protein phosphorylation.** *Nat Biotechnol* 2001, **19**:375-378.
  24. Oda Y, Nagasu T, Chait BT: **Enrichment analysis of phosphorylated proteins as a tool for probing the phosphoproteome.** *Nat Biotechnol* 2001, **19**:379-382.
  25. Ficarro SB, McClelland ML, Stukenberg PT, Burke DJ, Ross MM, Shabanowitz J, Hunt DF, White FM: **Phosphoproteome analysis by mass spectrometry and its application to *Saccharomyces cerevisiae*.** *Nat Biotechnol* 2002, **20**:301-305.
  26. Geng M, Zhang X, Bina M, Regnier F: **Proteomics of glycoproteins based on affinity selection of glycopeptides from tryptic digests.** *J Chromatogr B Biomed Sci Appl* 2001, **752**:293-306.
  27. Yao X, Freas A, Ramirez J, Demirev PA, Fenselau C: **Proteolytic  $^{18}\text{O}$  labeling for comparative proteomics: model studies with two serotypes of adenovirus.** *Anal Chem* 2001, **73**:2836-2842.
  28. Stewart II, Thomson T, Figeys D:  **$^{18}\text{O}$  labeling: a tool for proteomics.** *Rapid Commun Mass Spectrom* 2001, **15**:2456-2465.
  29. Conrads TP, Alving K, Veenstra TD, Belov ME, Anderson GA, Anderson DJ, Lipton MS, Pasa-Tolic L, Udseth HR, Chrisler WB *et al.*: **Quantitative analysis of bacterial and mammalian proteomes using a combination of cysteine affinity tags and  $^{15}\text{N}$ -metabolic labeling.** *Anal Chem* 2001, **73**:2132-2139.
  30. Oda Y, Huang K, Cross FR, Cowburn D, Chait BT: **Accurate quantitation of protein expression and site-specific phosphorylation.** *Proc Natl Acad Sci USA* 1999, **96**:6591-6596.
  31. Washburn MP, Ulaszek R, Deciu C, Schieltz DM, Yates JR III: **Analysis of quantitative proteomic data generated via multidimensional protein identification technology.** *Anal Chem* 2002, **74**:1650-1657.
  32. Shi SD, Hendrickson CL, Marshall AG: **Counting individual sulfur atoms in a protein by ultrahigh-resolution Fourier transform ion cyclotron resonance mass spectrometry: experimental resolution of isotopic fine structure in proteins.** *Proc Natl Acad Sci USA* 1998, **95**:11532-11537.
  33. Ong SE, Blagoev B, Kratchmarova I, Kristensen DB, Steen H, Pandey A, Mann M: **Stable isotope labeling by amino acids in cell culture, SILAC, as a simple and accurate approach to expression proteomics.** *Mol Cell Proteomics* 2002, **1**:376-386.
- Stable isotope labeling was applied to mammalian cells by *in vivo* incorporation of specific amino acids during cell culture.
34. Martinovic S, Veenstra TD, Anderson GA, Pasa-Tolic L, Smith RD: **Selective incorporation of isotopically labeled amino acids for identification of intact proteins on a proteome-wide level.** *J Mass Spectrom* 2002, **37**:99-107.
  35. Zhu H, Pan S, Gu S, Bradbury EM, Chen X: **Amino acid residue specific stable isotope labeling for quantitative proteomics.** *Rapid Commun Mass Spectrom* 2002, **16**:2115-2123.
  36. Zhu H, Hunter TC, Pan S, Yau PM, Bradbury EM, Chen X: **Residue-specific mass signatures for the efficient detection of protein modifications by mass spectrometry.** *Anal Chem* 2002, **74**:1687-1694.
  37. Cagney G, Emili A: ***De novo* peptide sequencing and quantitative profiling of complex protein mixtures using mass-coded abundance tagging.** *Nat Biotechnol* 2002, **20**:163-170.
  38. Keller A, Nesvizhskii AI, Kolker E, Aebersold R: **Empirical statistical model to estimate the accuracy of peptide identifications made by MS/MS and database search.** *Anal Chem* 2002, **74**:5383-5392.
  39. Griffin TJ, Han DK, Gygi SP, Rist B, Lee H, Aebersold R, Parker KC: **Toward a high-throughput approach to quantitative proteomic analysis: expression-dependent protein identification by mass spectrometry.** *J Am Soc Mass Spectrom* 2001, **12**:1238-1246.
  40. Yergey AL, Coorsen JR, Backlund PS Jr, Blank PS, Humphrey GA, Zimmerberg J, Campbell JM, Vestal ML: ***De novo* sequencing of peptides using MALDI/TOF-TOF.** *J Am Soc Mass Spectrom* 2002, **13**:784-791.
  41. Medzihradszky KF, Campbell JM, Baldwin MA, Fallick AM, Juhasz P, Vestal ML, Burlingame AL: **The characteristics of peptide collision-induced dissociation using a high-performance MALDI-TOF/TOF tandem mass spectrometer.** *Anal Chem* 2000, **72**:552-558.
  42. Lee H, Griffin TJ, Gygi SP, Rist B, Aebersold R: **Development of a multiplexed microcapillary liquid chromatography system for high-throughput proteome analysis.** *Anal Chem* 2002, **74**:4353-4360.
  43. Krutchinsky AN, Kalkum M, Chait BT: **Automatic identification of proteins with a MALDI-quadrupole ion trap mass spectrometer.** *Anal Chem* 2001, **73**:5066-5077.
  44. Witzmann FA, Li J: **Cutting-edge technology. II. Proteomics: core technologies and applications in physiology.** *Am J Physiol Gastrointest Liver Physiol* 2002, **282**:G735-G741.
  45. Figeys D: **Proteomics approaches in drug discovery.** *Anal Chem* 2002, **74**:412A-419A.